

# Alcotest 7110 Calibration Record

## Equipment

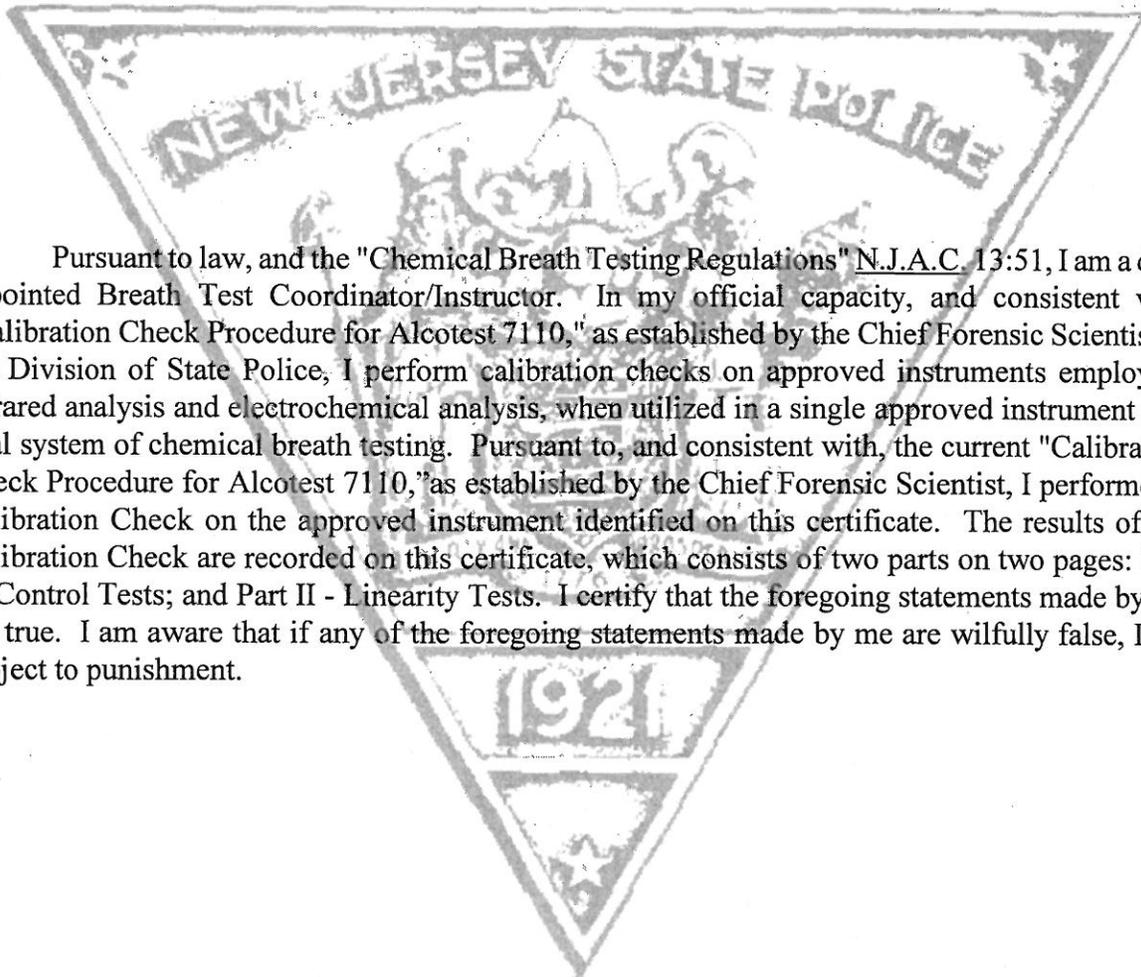
Alcotest 7110 MKIII-C  
Serial No.: ARTL-0005  
Location: PLAINSBORO TOWNSHIP PD  
Calibration File No.: 01186 Calib. Date: 09/05/2012 Calib. No.: 00021  
Certification File No.: 01115 Cert. Date: 04/03/2012 Cert. No.: 00014  
Linearity File No.: 01116 Lin. Date: 04/03/2012 Lin. No.: 00014  
Solution File No.: 01180 Soln. Date: 08/24/2012 Soln. No.: 00146  
Sequential File No.: 01186 File Date: 09/05/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064  
Control Solution %: 0.100% Expires: 02/20/2014  
Solution Control Lot: 12B099 Bottle No.: 0889

## Coordinator

Last Name: GONCALVES First Name: MICHELLE MI: L  
Signature: Det I Glens # 6040 Badge No.: 6040  
Date: 09/05/2012

\*Black Key Temperature Probe Serial.....# DDMBP9-0002 Me  
\*Digital NIST Temperature Measuring System Serial.....# 122172176 W



Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

### Equipment

Alcotest 7110 MKIII-C  
Location: PLAINSBORO TOWNSHIP PD  
Serial No.: ARTL-0005  
Calibration File No.: 01186  
Calib. Date: 09/05/2012  
Calib. No.: 00021  
Certification File No.: 01187  
Cert. Date: 09/05/2012  
Cert. No.: 00015  
Linearity File No.: 01116  
Lin. Date: 04/03/2012  
Lin. No.: 00014  
Solution File No.: 01180  
Soln. Date: 08/24/2012  
Soln. No.: 00146  
Sequential File No.: 01187  
File Date: 09/05/2012

Calibrating Unit: WET  
Model No.: CU-34  
Serial No.: DDUF S3-0064  
Control Solution %: 0.100%  
Expires: 02/20/2014  
Solution Control Lot: 12B099  
Bottle No.: 0889

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:05D		
Control 1 EC	0.099%	10:05D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:05D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06D		
Control 2 EC	0.099%	10:06D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:06D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:07D		
Control 3 EC	0.099%	10:08D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:08D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:08D		

All tests within acceptable tolerance.

### Coordinator

Last Name: GONCALVES First Name: MICHELLE MI L

Signature: 

Badge No.: 6040

Date: 09/05/2012

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTL-0005  
Location: PLAINSBORO TOWNSHIP PD  
Calibration File No.: 01186 Calib. Date: 09/05/2012 Calib. No.: 00021  
Certification File No.: 01187 Cert. Date: 09/05/2012 Cert. No.: 00015  
Linearity File No.: 01188 Lin. Date: 09/05/2012 Lin. No.: 00015  
Solution File No.: 01180 Soln. Date: 08/24/2012 Soln. No.: 00146  
Sequential File No.: 01188 File Date: 09/05/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0215  
Control Solution %: 0.040% Expires: 06/27/2013  
Solution Control Lot: 11F090 Bottle No.: 1243

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0193  
Control Solution %: 0.080% Expires: 06/30/2013  
Solution Control Lot: 11F091 Bottle No.: 0935

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0241  
Control Solution %: 0.160% Expires: 07/03/2013  
Solution Control Lot: 11G092 Bottle No.: 0448

Function	Result	Time	Temperature	Comment(s)
	%BAC <sub>c</sub>	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:20D		
Control 1 EC	0.041%	10:21D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.037%	10:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:22D		
Control 2 EC	0.040%	10:23D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.038%	10:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:24D		
Control 3 EC	0.080%	10:24D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.079%	10:24D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:26D		
Control 4 EC	0.079%	10:26D	33.9°C	*** TEST PASSED ***
Control 4 IR	0.077%	10:26D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:28D		
Control 5 EC	0.159%	10:28D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.158%	10:28D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:30D		
Control 6 EC	0.159%	10:30D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.156%	10:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:32D		

All tests within acceptable tolerance.

### Coordinator

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: Det J. G. Alves # 6040

Badge No.: 6040

Date: 09/05/2012

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTL-0005  
 Location: PLAINSBORO TOWNSHIP PD  
 Calibration File No.: 01186 Calib. Date: 09/05/2012 Calib. No.: 00021  
 Certification File No.: 01187 Cert. Date: 09/05/2012 Cert. No.: 00015  
 Linearity File No.: 01188 Lin. Date: 09/05/2012 Lin. No.: 00015  
 Solution File No.: 01189 Soln. Date: 09/05/2012 Soln. No.: 00147  
 Sequential File No.: 01189 File Date: 09/05/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0064  
 Control Solution %: 0.100% Expires: 12/16/2012  
 Solution Control Lot: 10L084 Bottle No.: 0398

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:40D		
Control 1 EC	0.100%	11:40D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:40D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:41D		
Control 2 EC	0.100%	11:42D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:42D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:42D		
Control 3 EC	0.100%	11:43D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:43D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:43D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number DD5FP2-0396 (WRA)

**Changed By:**

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: Det I Golves #6040

Badge No.: 6040

Date: 09/05/2012



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DD4F53-0064

Certification Date

Technician

Re-Certification Due Date

1/17/12

DM

1/17/13

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

### CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDSEF2-0396

1/17/12

1/17/13

Probe Value

1.05

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

DM



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDWFS3-0241

Certification Date

Technician

Re-Certification Due Date

2/2/12

DM

2/2/13



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDWFS3-0215

Certification Date

Technician

Re-Certification Due Date

2/2/12

DM

2/2/13



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Serial Number:

Model: MARK IIA

DDX053-0193

Other: \_\_\_\_\_

Certification Date

Technician

Re-Certification Due Date

8-6-12

AS

8-6-13

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

### CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDMB P1-0002

2/3/12

2/3/13

Probe Value

102

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

AM



**Dräger**

**Alcotest® 7110 MKIII-C**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

SERIAL NUMBER:

5-12-2011

ARTL-0005

Draeger Safety Diagnostics, Inc.

AS



Calibration  
Certificate No. 1750.01

Calibration complies with ISO/IEC  
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-4269985

**Traceable® Certificate of Calibration for Digital Thermometer**

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Metsonford Road, Radnor, PA 19087  
Instrument Identification:

Model: 61220-601      S/N: 122172178      Manufacturer: Control Company

**Standards/Equipment:**

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-275	A9A237		
Digital Thermometer	B16815	6/06/12	B1606038
PRT Temperature Probe	01841	6/28/12	B1526085
Temperature Calibration Bath TC-256	B01375		
Thermistor Module	A27129	10/31/12	1000306945
Temperature Probe	157	11/13/12	6-BL72N-1-1
Temperature Calibration Bath TC-179	A45240		
Thermistor Module	A17118	2/01/13	1000311439
Temperature Probe	128	2/14/13	6-BN9WZ-27-1

**Certificate Information:**

Technician: 68      Procedure: CAL-08      Cal Date: 3/30/12      Cal Due: 3/30/14  
Test Conditions: 23.0°C      44.0 %RH      1012 mBar

**Calibration Data: (New Instrument)**

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		-0.000	-0.001	Y	-0.050	0.050	0.013	3.8:1
°C		N.A.		25.001	25.000	Y	24.951	25.051	0.014	3.8:1
°C		N.A.		60.000	59.999	Y	59.950	60.050	0.016	2.8:1
°C		N.A.		100.001	100.002	Y	99.951	100.051	0.018	2.8:1

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Reading(Rounded) + Tolerance; Date=MM/DD/YY

*Nicol Rodriguez*  
Nicol Rodriguez, Quality Manager

*Wallace Berry*  
Wallace Berry, Technical Manager

**Maintaining Accuracy:**

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

**Recalibration:**

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4485 Rex Road Friendswood, TX 77546 USA  
Phone 281 482-1714 Fax 281 482-8448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01605-2008-AQ-HOU-ANAB.  
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor
KIM GUADAGNO
Lt. Governor

PAULA T. DOW
Attorney General
COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 1/19/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10L084

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1185 to 0.1190 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 16, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Kenneth W. Kawalek

Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 24th day of January, 2011.

Handwritten signature of Linda L. Desantis
Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 Post Office Box 7068  
 West Trenton NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

KIM GUADAGNO  
 Lt. Governor

PAULA T. DOW  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.


MANUFACTURER: Dräger Safety, Inc. ANALYSIS DATE: 7/21/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11F090


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0478 to 0.0485 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13-51-3.4, of approved breath test instruments (N.J.A.C. 13-51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 27, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

  
 Kenneth W. Krawalek, M.S.  
 Assistant Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 1<sup>st</sup> day of August, 2011.

  
 Notary

Linda L. Deonnis  
 Notary Public, New Jersey  
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





CHRIS CHRISTIE  
Governor

KIM GUADAGNO  
Lt. Governor

State of New Jersey  
OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
Post Office Box 7068  
West Trenton NJ 08628-0068  
(609) 882-2000

PAULA T. DOW  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Dreger Safety, Inc.

ANALYSIS DATE: 7/22/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11E091

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.096% to 0.097% grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13-51-3.4, of approved breath test instruments (N.J.A.C. 13-51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 30, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Kenneth W. Kwalek, M.S.  
Assistant Chief Forensic Scientist  
Division of State Police

Sworn to and subscribed before me this 1<sup>st</sup> day of August, 2011.

Notary

Linda L. DeLantis  
Notary Public, State of New Jersey  
My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON, NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

JEFFREY S. CHIESA  
 Attorney General

KIM GUADAGNO  
 Lt. Governor

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.

ANALYSIS DATE: 3/20/2012

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 12B099

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1207 to 0.1211 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 20, 2014.

As Forensic Scientist III for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Monica L. Tramontin  
 Forensic Scientist III  
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20<sup>th</sup> day of March, 2012.

Notary

MARY ELIZABETH MCLAUGHLIN  
 NOTARY PUBLIC OF NEW JERSEY  
 MY COMMISSION EXPIRES 12-24-2013



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 Post Office Box 7068  
 West Trenton NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

KIM GUADAGNO  
 Lt. Governor

PAULA T. DOW  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 7/25/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11G092


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1917 to 0.1927 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 3, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

  
 Kenneth W. Kowalek, M.S.  
 Assistant Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 1<sup>st</sup> day of August, 2011.

  
 Notary

Linda L. Demaris  
 Notary Public, New Jersey  
 My Commission Expires 9-11-14



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





# CERTIFICATE

This is to certify that

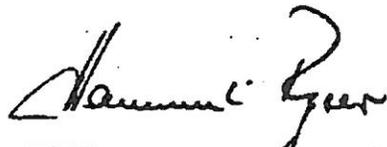
**Michelle Goncalves**

has successfully completed the two day Draeger Safety Diagnostics, Inc. Alcohol Coordinator Training Course on the New Jersey specific Alcotest® 7110 MKIII-C and is hereby certified as a qualified

**Operator Trainer and  
Maintenance Technician**

Completion of this course qualifies this individual to train and certify Operators in the proper use and operation as well as perform Preventive Maintenance on the New Jersey specific Alcotest® 7110 MKIII-C.

Date: March 14, 2012

  
\_\_\_\_\_  
Instructor: Hansueli Ryser

**Dräger**



CHRIS CHRISTIE  
Governor

KIM GUADAGNO  
Lieutenant Governor

*State of New Jersey*  
OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF CRIMINAL JUSTICE  
PO BOX 085  
TRENTON, NJ 08625-0085  
TELEPHONE: (609) 984-6300

JEFFREY S. CHIESA  
Attorney General

STEPHEN J. TAYLOR  
Director

March 23, 2012

Col. Joseph R. Fuentes, Superintendent  
Division of State Police  
Division Headquarters  
P.O. Box 7068  
West Trenton, New Jersey 08628

Re: Breath Test Coordinator/Instructor, Certification -  
Detective I Michelle L. Goncalves #6040

Dear Col. Fuentes:

Pursuant to the provisions of *N.J.A.C.* 13:51-2.1 (b) and (c), as adopted and promulgated under the provisions of *N.J.S.A.* 39:4-50.3, 39:3-10.25 and 12:7-56, I hereby approve Detective I Michelle L. Goncalves #6040, as a duly certified Breath Test Coordinator/Instructor. This approval is effective immediately.

Very truly yours,

Jeffrey S. Chiesa  
Attorney General

- c. Detective I Michelle L. Goncalves, Alcohol/Drug Test Unit, Division of State Police  
DSFC Patrick Guilfooy, Unit Head, Alcohol/Drug Test Unit, Division of State Police ✓



DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that  
**Michelle L. McKelvey**  
IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL ANALYSIS PURSUANT TO CHAPTER 146 OF THE LAWS OF 1966 IN THE OPERATION OF THE **Breathalyzer**  
A METHOD TO DETERMINE INTOXICATION,  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS **16th** DAY OF **Aug.**  
TWO THOUSAND AND **04**

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES Feb. 3-7-2003  
Refresher Course

DATE	PLACE	INSTRUCTOR
1. <u>10/1/05</u>	<u>OCSPA</u>	<u>[Signature]</u>
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 283B (Rev. 05/02)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that  
**MICHELLE L. MCKELVEY**  
NEW JERSEY STATE POLICE  
IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL ANALYSIS PURSUANT TO CHAPTER 146 OF THE LAWS OF 1966 IN THE OPERATION OF THE **ALCOHOL TEST 7110 MKIII-C**  
A METHOD TO DETERMINE INTOXICATION,  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS **10th** DAY OF **August**  
TWO THOUSAND AND **FIVE**

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_  
Refresher Course

DATE	PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 283B (Rev. 05/02)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that  
**Michelle L. Gonçalves**  
New Jersey State Police  
IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL ANALYSIS PURSUANT TO CHAPTER 146 OF THE LAWS OF 1966 IN THE OPERATION OF THE **ALCOHOL 7110 MKIII-C**  
A METHOD TO DETERMINE INTOXICATION,  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS **15th** DAY OF **December**  
TWO THOUSAND AND **EIGTEEN**

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_  
Refresher Course

DATE	PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 283B (Rev. 05/02)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that  
**Michelle Gonçalves**  
New Jersey State Police  
IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL ANALYSIS PURSUANT TO CHAPTER 146 OF THE LAWS OF 1966 IN THE OPERATION OF THE **Breath Test Coordinator/Instructor**  
A METHOD TO DETERMINE INTOXICATION,  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS **23rd** DAY OF **March**  
TWO THOUSAND AND **Twelve**

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_  
Refresher Course

DATE	PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 283B (Rev. 05/02)