

Alcotest 7110 Calibration Record

Equipment


Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 01042
Calib. Date: 11/16/2011
Calib. No.: 00019
Certification File No.: 00954
Cert. Date: 05/19/2011
Cert. No.: 00012
Linearity File No.: 00955
Lin. Date: 05/19/2011
Lin. No.: 00012
Solution File No.: 01034
Soln. Date: 10/28/2011
Soln. No.: 00132
Sequential File No.: 01042
File Date: 11/16/2011

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 10I082
Model No.: CU-34
Serial No.: DDUF S3-0065
Expires: 09/09/2012
Bottle No.: 1068

Coordinator

Last Name: GIBSON
First Name: MICHAEL
MI: P.
Signature: *Mr. Michael P. Gibson #6353*
Badge No.: 6353
Date: 11/16/2011

*Black Key Temperature Probe Serial.....# DDLHP1-0073 *(MPS)*
*Digital NIST Temperature Measuring System Serial.....# 101686537 *(MPS)*

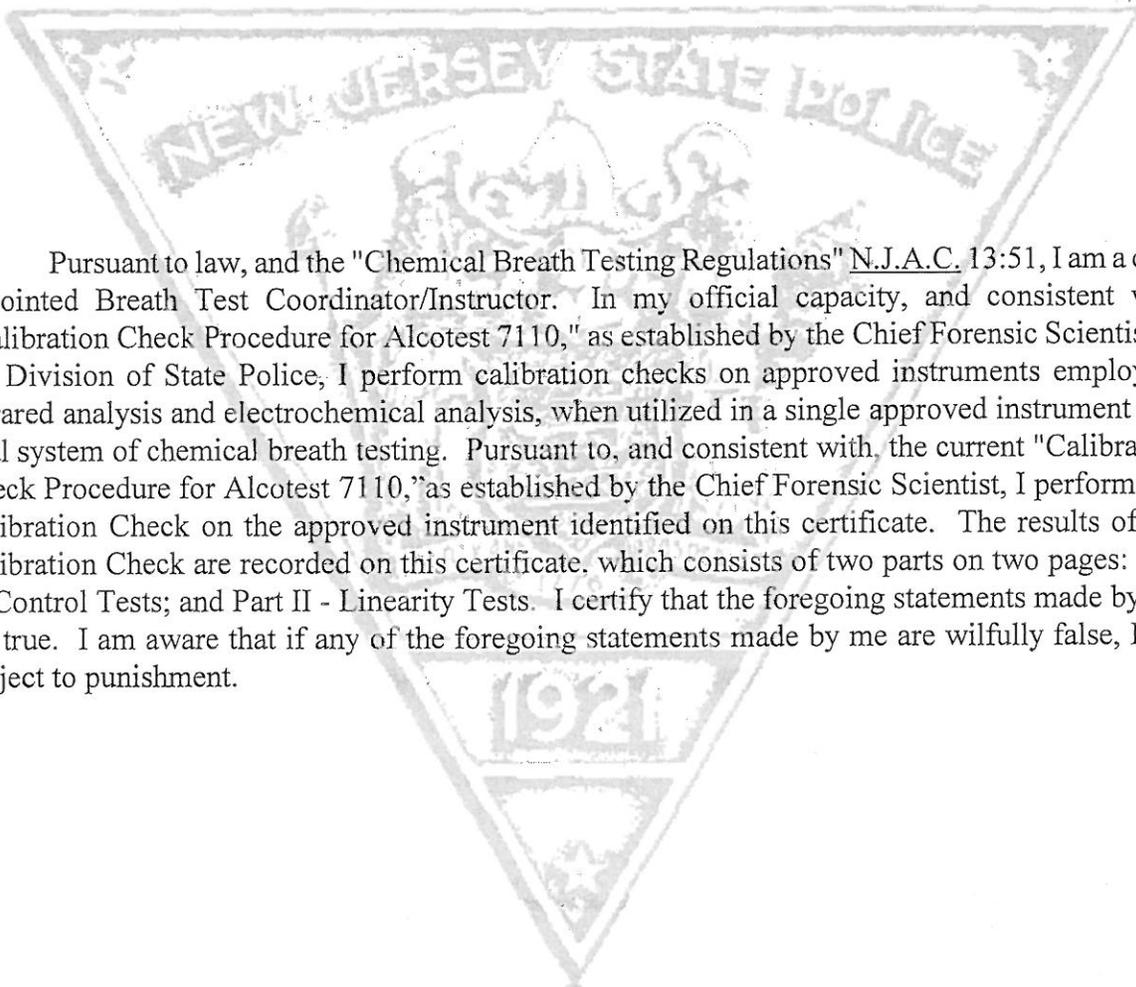

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01042 Calib. Date: 11/16/2011 Calib. No.: 00019
Certification File No.: 01043 Cert. Date: 11/16/2011 Cert. No.: 00013
Linearity File No.: 00955 Lin. Date: 05/19/2011 Lin. No.: 00012
Solution File No.: 01034 Soln. Date: 10/28/2011 Soln. No.: 00132
Sequential File No.: 01043 File Date: 11/16/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 09/09/2012
Solution Control Lot: 10I082 Bottle No.: 1068

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 10:25S | | |
| Control 1 EC | 0.100% | 10:25S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 10:25S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:26S | | |
| Control 2 EC | 0.100% | 10:26S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.099% | 10:26S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:27S | | |
| Control 3 EC | 0.099% | 10:28S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 10:28S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:28S | | |

All tests within acceptable tolerance.

Coordinator

Last Name: GIBSON

First Name: MICHAEL

MI: P.

Signature: 

Badge No.: 6353

Date: 11/16/2011

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0005
Location: PLAINSBORO TOWNSHIP PD
Calibration File No.: 01042 Calib. Date: 11/16/2011 Calib. No.: 00019
Certification File No.: 01043 Cert. Date: 11/16/2011 Cert. No.: 00013
Linearity File No.: 01044 Lin. Date: 11/16/2011 Lin. No.: 00013
Solution File No.: 01034 Soln. Date: 10/28/2011 Soln. No.: 00132
Sequential File No.: 01044 File Date: 11/16/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0187
Control Solution %: 0.040% Expires: 01/12/2012
Solution Control Lot: 10A073 Bottle No.: 0290

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAE-0021
Control Solution %: 0.080% Expires: 01/15/2012
Solution Control Lot: 10A074 Bottle No.: 0538

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDBN-0007
Control Solution %: 0.160% Expires: 01/21/2012
Solution Control Lot: 10A075 Bottle No.: 1188

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 10:39S | | |
| Control 1 EC | 0.042% | 10:39S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.039% | 10:39S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:41S | | |
| Control 2 EC | 0.042% | 10:41S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.040% | 10:41S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:43S | | |
| Control 3 EC | 0.081% | 10:43S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.080% | 10:43S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:45S | | |
| Control 4 EC | 0.081% | 10:45S | 34.0°C | *** TEST PASSED *** |
| Control 4 IR | 0.080% | 10:45S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:47S | | |
| Control 5 EC | 0.162% | 10:47S | 34.0°C | *** TEST PASSED *** |
| Control 5 IR | 0.161% | 10:47S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:49S | | |
| Control 6 EC | 0.160% | 10:49S | 34.0°C | *** TEST PASSED *** |
| Control 6 IR | 0.156% | 10:49S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:51S | | |

All tests within acceptable tolerance.

Coordinator

Last Name: GIBSON

First Name: MICHAEL

MI: P.

Signature: Jpr. # Michael P. Gibson #0353

Badge No.: 6353

Date: 11/16/2011

Calibrating Unit

New Standard Solution Report

| | | | |
|-------------------------|------------------------|--------------|--------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: | ARTL-0005 |
| Location: | PLAINSBORO TOWNSHIP PD | | |
| Calibration File No.: | 01042 | Calib. Date: | 11/16/2011 |
| Certification File No.: | 01043 | Cert. Date: | 11/16/2011 |
| Linearity File No.: | 01044 | Lin. Date: | 11/16/2011 |
| Solution File No.: | 01045 | Soln. Date: | 11/16/2011 |
| Sequential File No.: | 01045 | File Date: | 11/16/2011 |
| | | Calib. No.: | 00019 |
| | | Cert. No.: | 00013 |
| | | Lin. No.: | 00013 |
| | | Soln. No.: | 00133 |
| | | | |
| Calibrating Unit: | WET | Model No.: | CU-34 |
| Control Solution %: | 0.100% | Serial No.: | DDUF S3-0065 |
| Solution Control Lot: | 10L084 | Expires: | 12/16/2012 |
| | | Bottle No.: | 0381 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 11:55S | | |
| Control 1 EC | 0.101% | 11:56S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 11:56S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:56S | | |
| Control 2 EC | 0.101% | 11:57S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.099% | 11:57S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:57S | | |
| Control 3 EC | 0.101% | 11:58S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.101% | 11:58S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:59S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDUIPZ-144 MPJ

Changed By:

Last Name: GIBSON

First Name: MICHAEL

MI: P.

Signature: Tpr. # Michael P. Gibbon # 6353

Badge No.: 6353

Date: 11/16/2011



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDXDS3-0187

Certification Date


6-3-11

Technician

MM

Re-Certification Due Date

6-3-12



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDAE-0021

Certification Date

6-3-11

Technician

MM

Re-Certification Due Date

6-3-12



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDBN-0007

Certification Date

02-11-11

Technician

[Signature]

Re-Certification Due Date

02-11-12

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDLHPI-0073

Certification date:

February 7, 2011

Next Certification due:

February 7, 2012

Probe Value

104

Draeger Safety Diagnostics, Inc.
Technical Service Department

[Signature]



Calibration complies with ISO 9001
ISO/IEC 17025 AND ANSI/NCCL Z540-1



Cert. No.: 4000-2925216

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, P.O. Box 2158, Secaucus, NJ 07094 U.S.A.

Instrument Identification:

Model: 61220-601 S/N: 101686537 Manufacturer: Control Company

Standards/Equipment:

| Description | Serial Number | Due Date | NIST Traceable Reference |
|-------------------------------------|---------------|----------|--------------------------|
| Temperature Calibration Bath TC-179 | A45240 | | |
| Thermistor Module | A17118 | 11/19/10 | A9B21010 |
| Temperature Probe | 128 | 12/10/10 | A9B23079 |
| Temperature Calibration Bath TC-231 | A79341 | | |
| Temperature Probe | 3039 | 12/10/10 | A9B23080-1 |
| Temperature Calibration Bath TC-218 | A73332 | | |
| Thermistor Module | A27129 | 7/09/10 | 1000264338 |
| Temperature Probe | 5202 | 3/11/11 | B0310050 |
| Temperature Calibration Bath TC-256 | B01375 | | |
| Temperature Probe | 157 | 7/27/10 | A9708011-4 |

Certificate Information:

Technician: 68 Procedure: CAL-06 Cal Date: 5/17/10 Cal Due: 5/17/12
Test Conditions: 23.5°C 47.0 %RH 1017 mBar

Calibration Data: (New Instrument)

| Unit(s) | Nominal | As Found | In Tol | Nominal | As Left | In Tol | Min | Max | ±uc | TUR |
|---------|---------|----------|--------|---------|---------|--------|--------|---------|-------|-------|
| °C | | N.A. | | 0.002 | 0.000 | Y | -0.048 | 0.052 | 0.013 | 3.8:1 |
| °C | | N.A. | | 25.001 | 24.999 | Y | 24.951 | 25.051 | 0.013 | 3.8:1 |
| °C | | N.A. | | 60.002 | 60.003 | Y | 59.952 | 60.052 | 0.018 | 2.8:1 |
| °C | | N.A. | | 100.001 | 100.001 | Y | 99.951 | 100.051 | 0.013 | 3.8:1 |

This Instrument was calibrated using instruments Traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±uc=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = Nominal(Rounded) - Tolerance; Max = Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Wallace Berry
Wallace Berry, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

PAULA T. DOW
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 9/23/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10I082

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1190 to 0.1194 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 9, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Kenneth W. Kawalek, M.S.
Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 28th day of September, 2010.

Handwritten signature of Linda L. Desantis
Linda L. Desantis
Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





CHRIS CHRISTIE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

PAULA T. DOW
Acting Attorney General
COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.


MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 2/2/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10A073


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0479 to 0.0481 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 12, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

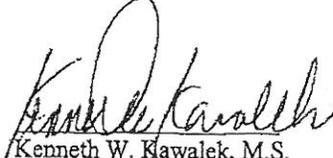
Kenneth W. Klawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of February, 2010.


Notary

Linda L. Deanda
Notary Public, New Jersey
Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

PAULA T. DOW
 Acting Attorney General
 COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. **ANALYSIS DATE:** 2/3/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10A074

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0954 to 0.0958 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 15, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Kenneth W. Kawalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 19th day of February, 2010.

Notary



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





CHRIS CHRISTIE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

PAULA T. DOW
Acting Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. **ANALYSIS DATE:** 2/4/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10A075


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1913 to 0.1919 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 21, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of February, 2010.


Notary



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

PAULA T. DOW
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 1/19/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10L084

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1185 to 0.1190 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 16, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 24th day of January, 2011.

Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Michael P. Gibson
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C** A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 14th DAY OF June TWO THOUSAND AND FIVE

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

| DATE | Refresher Course PLACE | INSTRUCTOR |
|------------|------------------------|------------|
| 1. 12/3/07 | OCPA | Wm Woods |
| 2. 3-13-09 | BCPA | Wm Woods |
| 3. 2-3-11 | OCPA | Wm Woods |
| 4. _____ | _____ | _____ |
| 5. _____ | _____ | _____ |
| 6. _____ | _____ | _____ |
| 7. _____ | _____ | _____ |
| 8. _____ | _____ | _____ |
| 9. _____ | _____ | _____ |

S.P. 2938 (Rev. 06/03)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Michael Gibson
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE **Breath Test Coordinator/Instructor** A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 10th DAY OF June TWO THOUSAND AND Eleven

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

| DATE | Refresher Course PLACE | INSTRUCTOR |
|----------|------------------------|------------|
| 1. _____ | _____ | _____ |
| 2. _____ | _____ | _____ |
| 3. _____ | _____ | _____ |
| 4. _____ | _____ | _____ |
| 5. _____ | _____ | _____ |
| 6. _____ | _____ | _____ |
| 7. _____ | _____ | _____ |
| 8. _____ | _____ | _____ |
| 9. _____ | _____ | _____ |

S.P. 2938 (Rev. 03/10)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

MICHAEL P. GIBSON
NEW JERSEY STATE POLICE

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE **BREATHALYZER** A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 2nd DAY OF October TWO THOUSAND AND FOUR

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 07/21 TO 07/25/2003

| DATE | Refresher Course PLACE | INSTRUCTOR |
|------------|------------------------|------------|
| 1. 7-14-06 | OCPA | CPotts |
| 2. _____ | _____ | _____ |
| 3. _____ | _____ | _____ |
| 4. _____ | _____ | _____ |
| 5. _____ | _____ | _____ |
| 6. _____ | _____ | _____ |
| 7. _____ | _____ | _____ |
| 8. _____ | _____ | _____ |
| 9. _____ | _____ | _____ |

S.P. 2938 (Rev. 02/03)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Michael P. Gibson
North Wildwood City Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE **Breathalyzer** A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 25th DAY OF July TWO THOUSAND AND 03

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

| DATE | Refresher Course PLACE | INSTRUCTOR |
|----------|------------------------|------------|
| 1. _____ | _____ | _____ |
| 2. _____ | _____ | _____ |
| 3. _____ | _____ | _____ |
| 4. _____ | _____ | _____ |
| 5. _____ | _____ | _____ |
| 6. _____ | _____ | _____ |
| 7. _____ | _____ | _____ |
| 8. _____ | _____ | _____ |
| 9. _____ | _____ | _____ |

S.P. 2938 (Rev. 06/03)

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48864, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

SERIAL NUMBER:

5-12-2011

ARTL-0005

Draeger Safety Diagnostics, Inc.



Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

NDUJ P2-144

Certification date:

7-28-11

Next Certification due:

7-28-12

Probe Value

106

Draeger Safety Diagnostics, Inc.
Technical Service Department

MM



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

NDUFS3-0065

Certification Date

7-28-11

Technician

MM

Re-Certification Due Date

7-28-12