

Alcotest 7110 Calibration Record

Equipment


Alcotest 7110 MKIII-C	Serial No.:	ARTL-0005
Location: PLAINSBORO TOWNSHIP PD		
Calibration File No.: 00497	Calib. Date: 07/28/2008	Calib. No.: 00008
Certification File No.: 00404	Cert. Date: 11/14/2007	Cert. No.: 00005
Linearity File No.: 00405	Lin. Date: 11/14/2007	Lin. No.: 00005
Solution File No.: 00492	Soln. Date: 07/20/2008	Soln. No.: 00068
Sequential File No.: 00497	File Date: 07/28/2008	
Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUF S3-0065
Control Solution %: 0.100%		Expires: 02/22/2009
Solution Control Lot: 07B045		Bottle No.: 0054

Coordinator

Last Name: SNYDER First Name: THOMAS MI: J.
Signature: TPR I Thomas J. Snyder #5792 Badge No.: 5792
Date: 07/28/2008

*Black Key Temperature Probe Serial# DDUNP2-229 JJS

*Ertco-Hart Digital Temperature Measuring System Serial# A29881 JJS

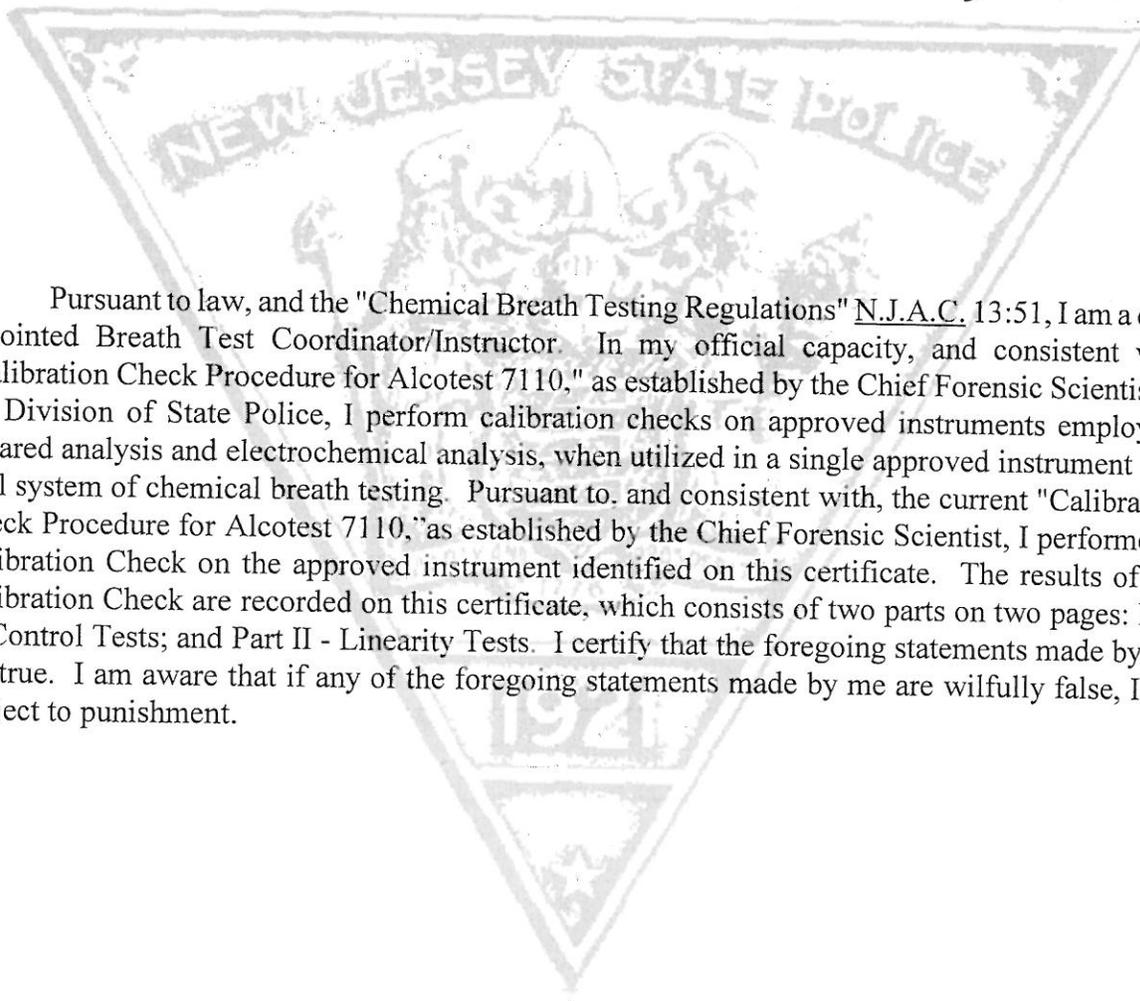

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 00497 Calib. Date: 07/28/2008 Calib. No.: 00008
Certification File No.: 00498 Cert. Date: 07/28/2008 Cert. No.: 00006
Linearity File No.: 00405 Lin. Date: 11/14/2007 Lin. No.: 00005
Solution File No.: 00492 Soln. Date: 07/20/2008 Soln. No.: 00068
Sequential File No.: 00498 File Date: 07/28/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUF S3-0065
Control Solution %: 0.100% Expires: 02/22/2009
Solution Control Lot: 07B045 Bottle No.: 0054

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:43D		
Control 1 EC	0.100%	13:44D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:45D		
Control 2 EC	0.098%	13:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:46D		
Control 3 EC	0.099%	13:46D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:47D		

All tests within acceptable tolerance.

Coordinator

Last Name: SNYDER First Name: THOMAS MI: J.
Signature: TPR. I Thomas J. Snyder #5792 Badge No.: 5792
Date: 07/28/2008

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment

Alcotest 7110 MKIII-C
Location: PLAINSBORO TOWNSHIP PD
Serial No.: ARTL-0005
Calibration File No.: 00497 Calib. Date: 07/28/2008 Calib. No.: 00008
Certification File No.: 00498 Cert. Date: 07/28/2008 Cert. No.: 00006
Linearity File No.: 00499 Lin. Date: 07/28/2008 Lin. No.: 00006
Solution File No.: 00492 Soln. Date: 07/20/2008 Soln. No.: 00068
Sequential File No.: 00499 File Date: 07/28/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0003
Control Solution %: 0.040% Expires: 01/26/2009
Solution Control Lot: 07A041 Bottle No.: 0126

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0184
Control Solution %: 0.080% Expires: 01/26/2009
Solution Control Lot: 07A042 Bottle No.: 0395

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDSC S3-0009
Control Solution %: 0.160% Expires: 01/26/2009
Solution Control Lot: 07A043 Bottle No.: 0082

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:07D		
Control 1 EC	0.041%	14:08D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	14:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:09D		
Control 2 EC	0.040%	14:10D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	14:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:11D		
Control 3 EC	0.081%	14:12D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	14:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:13D		
Control 4 EC	0.080%	14:14D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.081%	14:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:15D		
Control 5 EC	0.160%	14:16D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.160%	14:16D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:17D		
Control 6 EC	0.158%	14:18D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.159%	14:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:19D		

All tests within acceptable tolerance.

Coordinator

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: TR. I Thomas J. Snyder #5792

Badge No.: 5792

Date: 07/28/2008



Dräger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDRK 53-0003

Certification Date

Technician

Re-Certification Due Date

02-13-08

[Signature]

02-13-09



Dräger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDXDS3-0184

Certification Date

Technician

Re-Certification Due Date

02-13-08

[Signature]

02-13-09



Dräger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDSC 53-0009

Certification Date

Technician

Re-Certification Due Date

02-13-08

02-13-09

Dräger safety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).
The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDUN P2-229

02-12-08

02-12-09

Probe Value

102

Draeger Safety Diagnostics, Inc.
Technical Service Department



Ertco-Hart Digital Temperature Measuring System

REPORT OF CALIBRATION

This is to certify that the Ertco-Hart Digital Temperature Measuring System has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). Draeger Safety Diagnostics, Inc. (DSDI) recommends accuracy verification of the Ertco-Hart Digital Temperature Measuring System within 12 months of the certification date below, or sooner, according to your state specification.

DSDI equipment used for temperature

verification Serial Number: HH41 301316 / HH41 303176 / MERCURY THERMOMETER

Digital Units Serial Number: A29881

Probe Serial Number: 590802

Certification Date: 02-12-2008

Next Certification Due: 02-12-2009

At 34.00 °C digital unit displays 34.06 °C

Draeger Safety Diagnostics, Inc. Technician: 



JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

STUART RABNER
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. **ANALYSIS DATE:** 04/04/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07B045

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1222 to 0.1227 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 22, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 20th day of April, 2007.

Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

JON S. CORZINE
 Governor

ANNE MILGRAM
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 08/28/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08G058

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1228 to 0.1234 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 23, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tangare
 Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 22nd day of September 2008.

Notary

Linda L. DeSantis
 My Commission
 Expires Aug. 17, 2009





ION E. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

STUART RABNER
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 03/06/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07A041

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0483 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 29th day of March, 2007.

Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2008



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

JOHN S. CORZINE
 Governor

STUART RABNER
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. **ANALYSIS DATE:** 03/06/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07A042

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0965 to 0.0972 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare

Ajit R. Tungare
 Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 28th day of March, 2007.

Linda L. DeSantis
 Notary

Linda L. DeSantis
 My Commission
 Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

STUART RABNER
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 03/06/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07A043

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1932 to 0.1938 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009

Ajit R. Tungare
Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 29th day of March, 2007.

Linda L. DeSantis
Notary



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

STUART RABNER
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 12/06/06

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 06K037

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1213 to 0.1216 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 17, 2008.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare (Handwritten signature)

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 10th day of January 2007.

Linda L. DeSantis (Handwritten signature)
Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Thomas J. Snyder
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 7110 MKIII-C A METHOD TO DETERMINE INTOXICATION. GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 17th DAY OF June TWO THOUSAND AND SIX

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

DATE	Refresher Course PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 01/06)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Thomas J. Snyder
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MKIII-C A METHOD TO DETERMINE INTOXICATION. GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 22nd DAY OF February TWO THOUSAND AND SIX

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

DATE	Refresher Course PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 01/06)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Thomas J. Snyder
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Breathalyzer A METHOD TO DETERMINE INTOXICATION. GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 11th DAY OF Aug. TWO THOUSAND AND 00

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>11-14-01</u>	<u>ACTC</u>	<u>[Signature]</u>
2. <u>5-5-03</u>	<u>OCPA</u>	<u>[Signature]</u>
3. <u>4-4-05</u>	<u>ACTC</u>	<u>[Signature]</u>
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

SP-293B (Rev. 11/99)

Drägersafety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDUJP2-144


04-16-08


04-16-09

Probe Value

106

Draeger Safety Diagnostics, Inc.
Technical Service Department





Drägersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST[®] CU34

Model: MARK IIA

Other: _____

Serial Number:

DDVF 53-0065

Certification Date

Technician

Re-Certification Due Date

APR. 18/2008

TG

APR. 18/2009

Drägersafety

Alcotest[®] 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

01/22/2007

SERIAL NUMBER:

ARTL-0005

Draeger Safety Diagnostics, Inc.
Durango, CO

LRD